

Fig. 1.

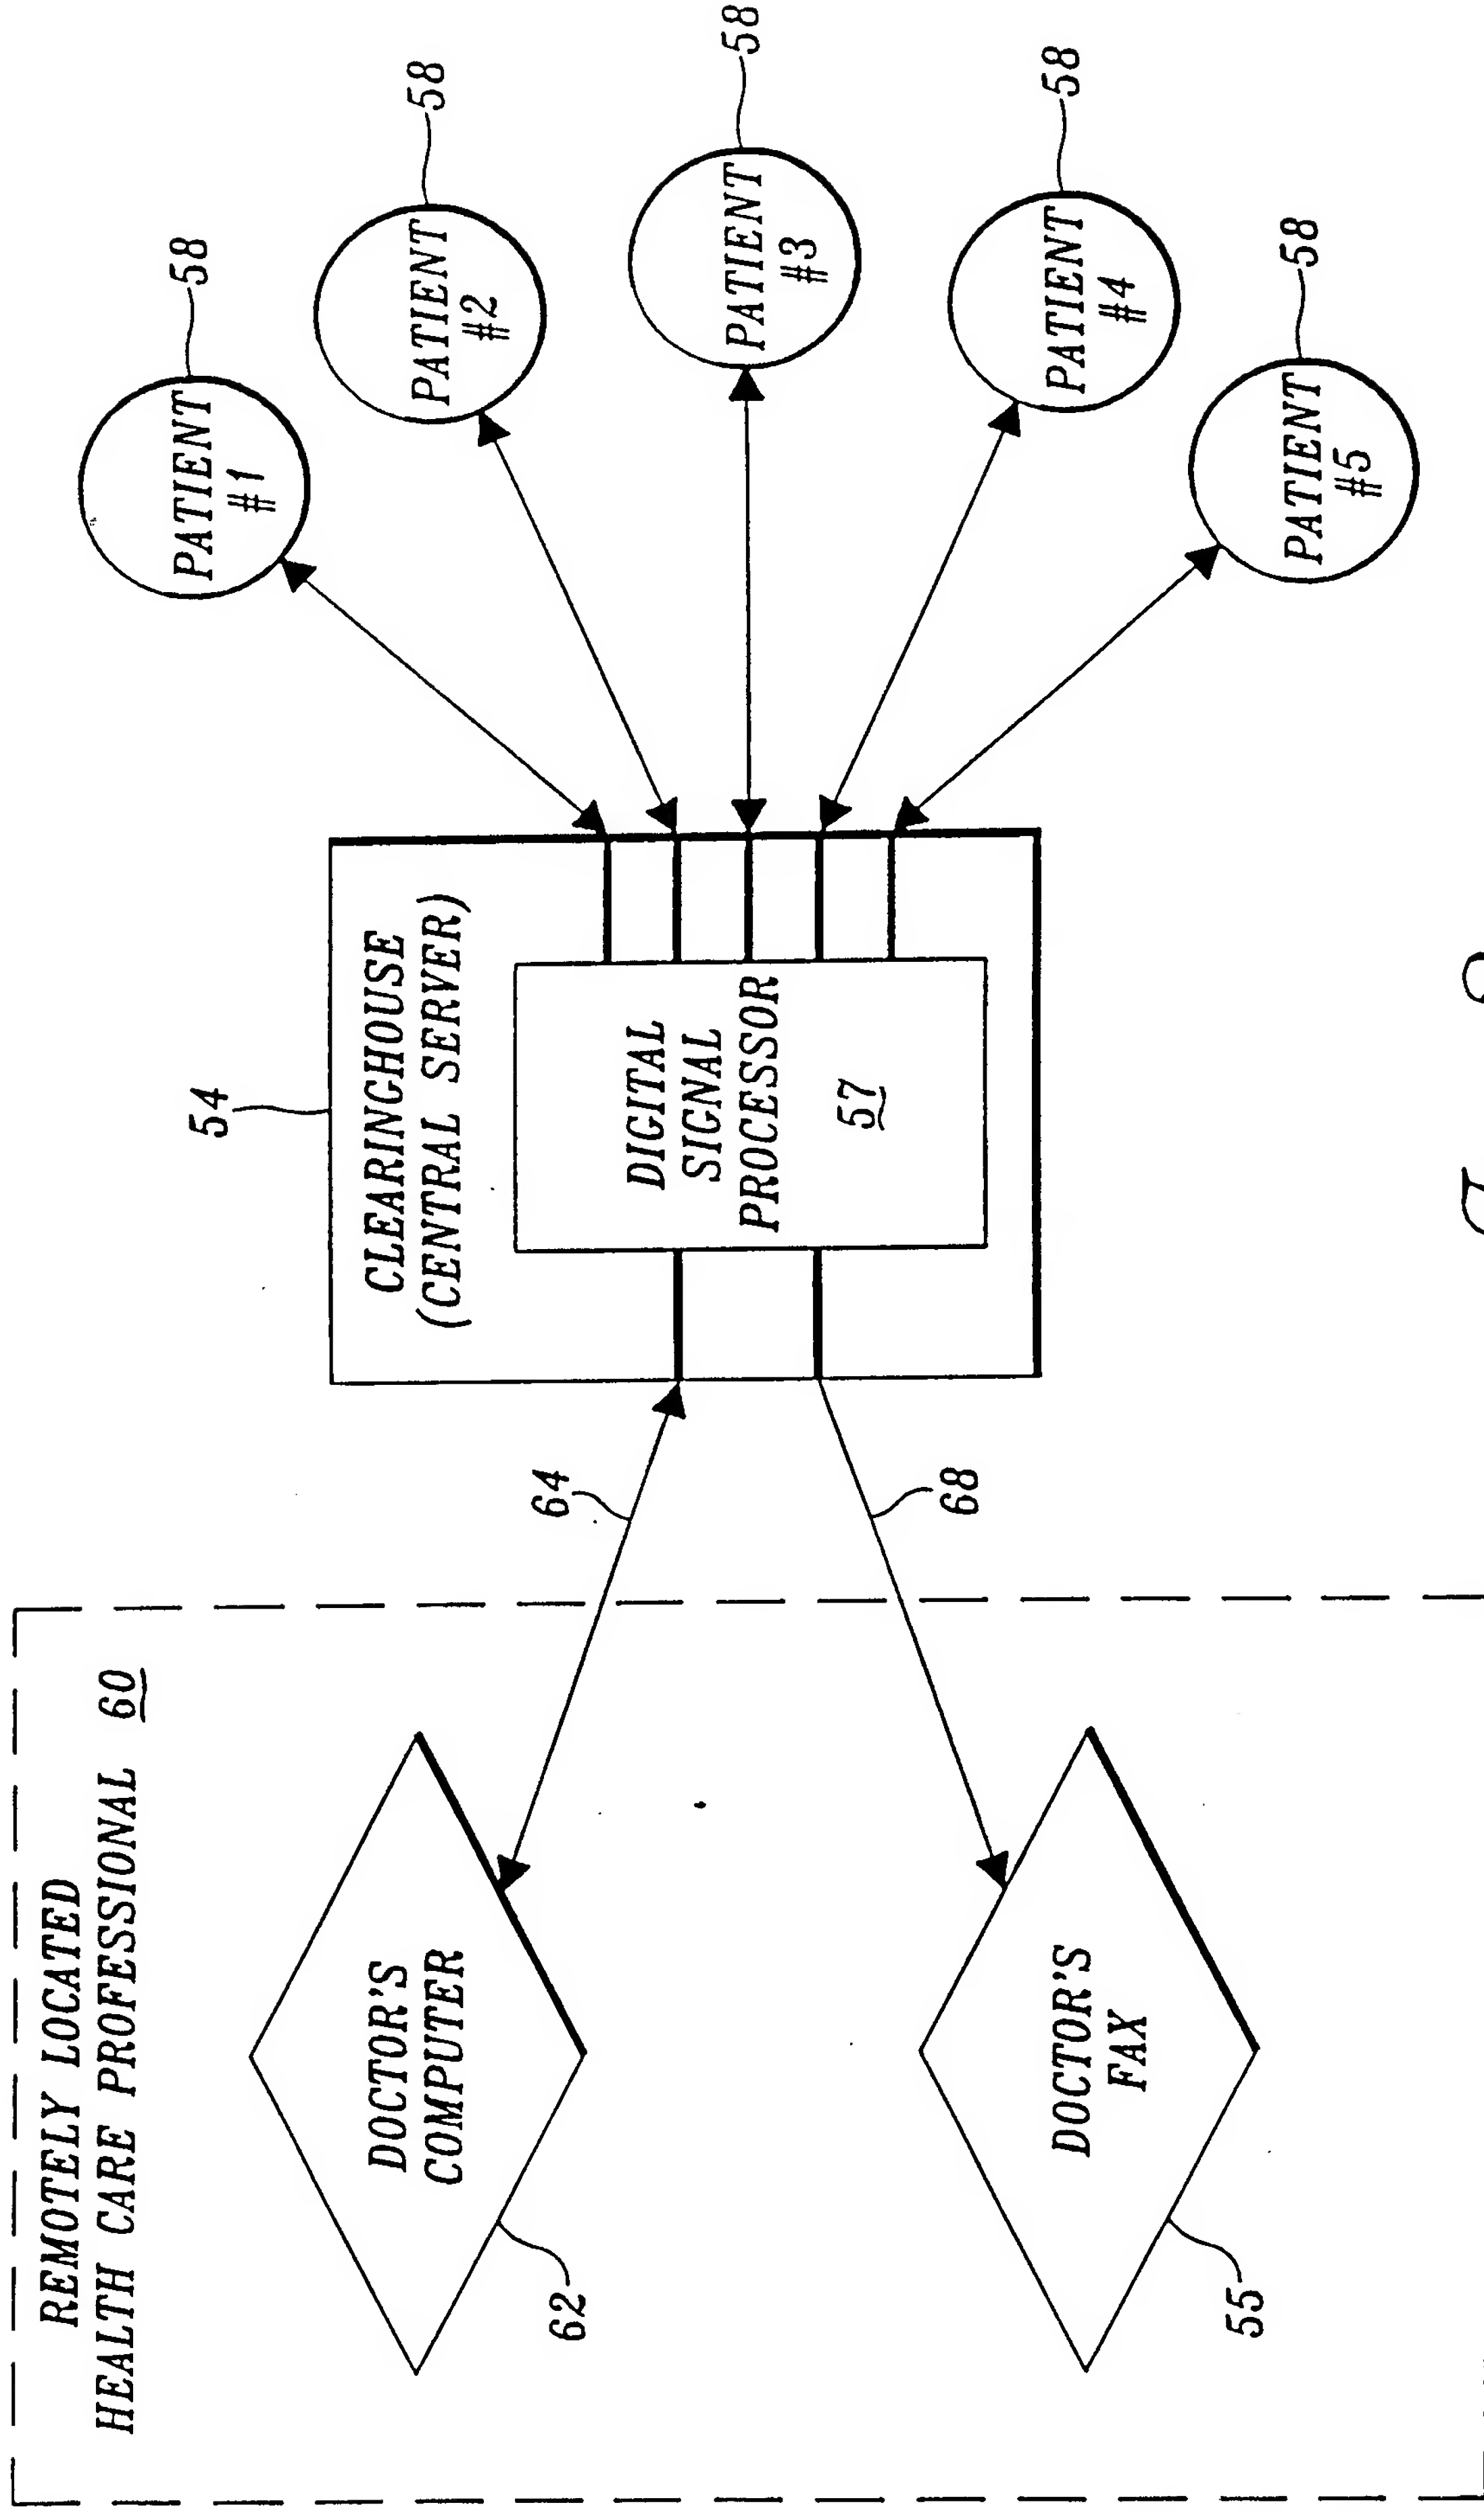


Fig. 2.

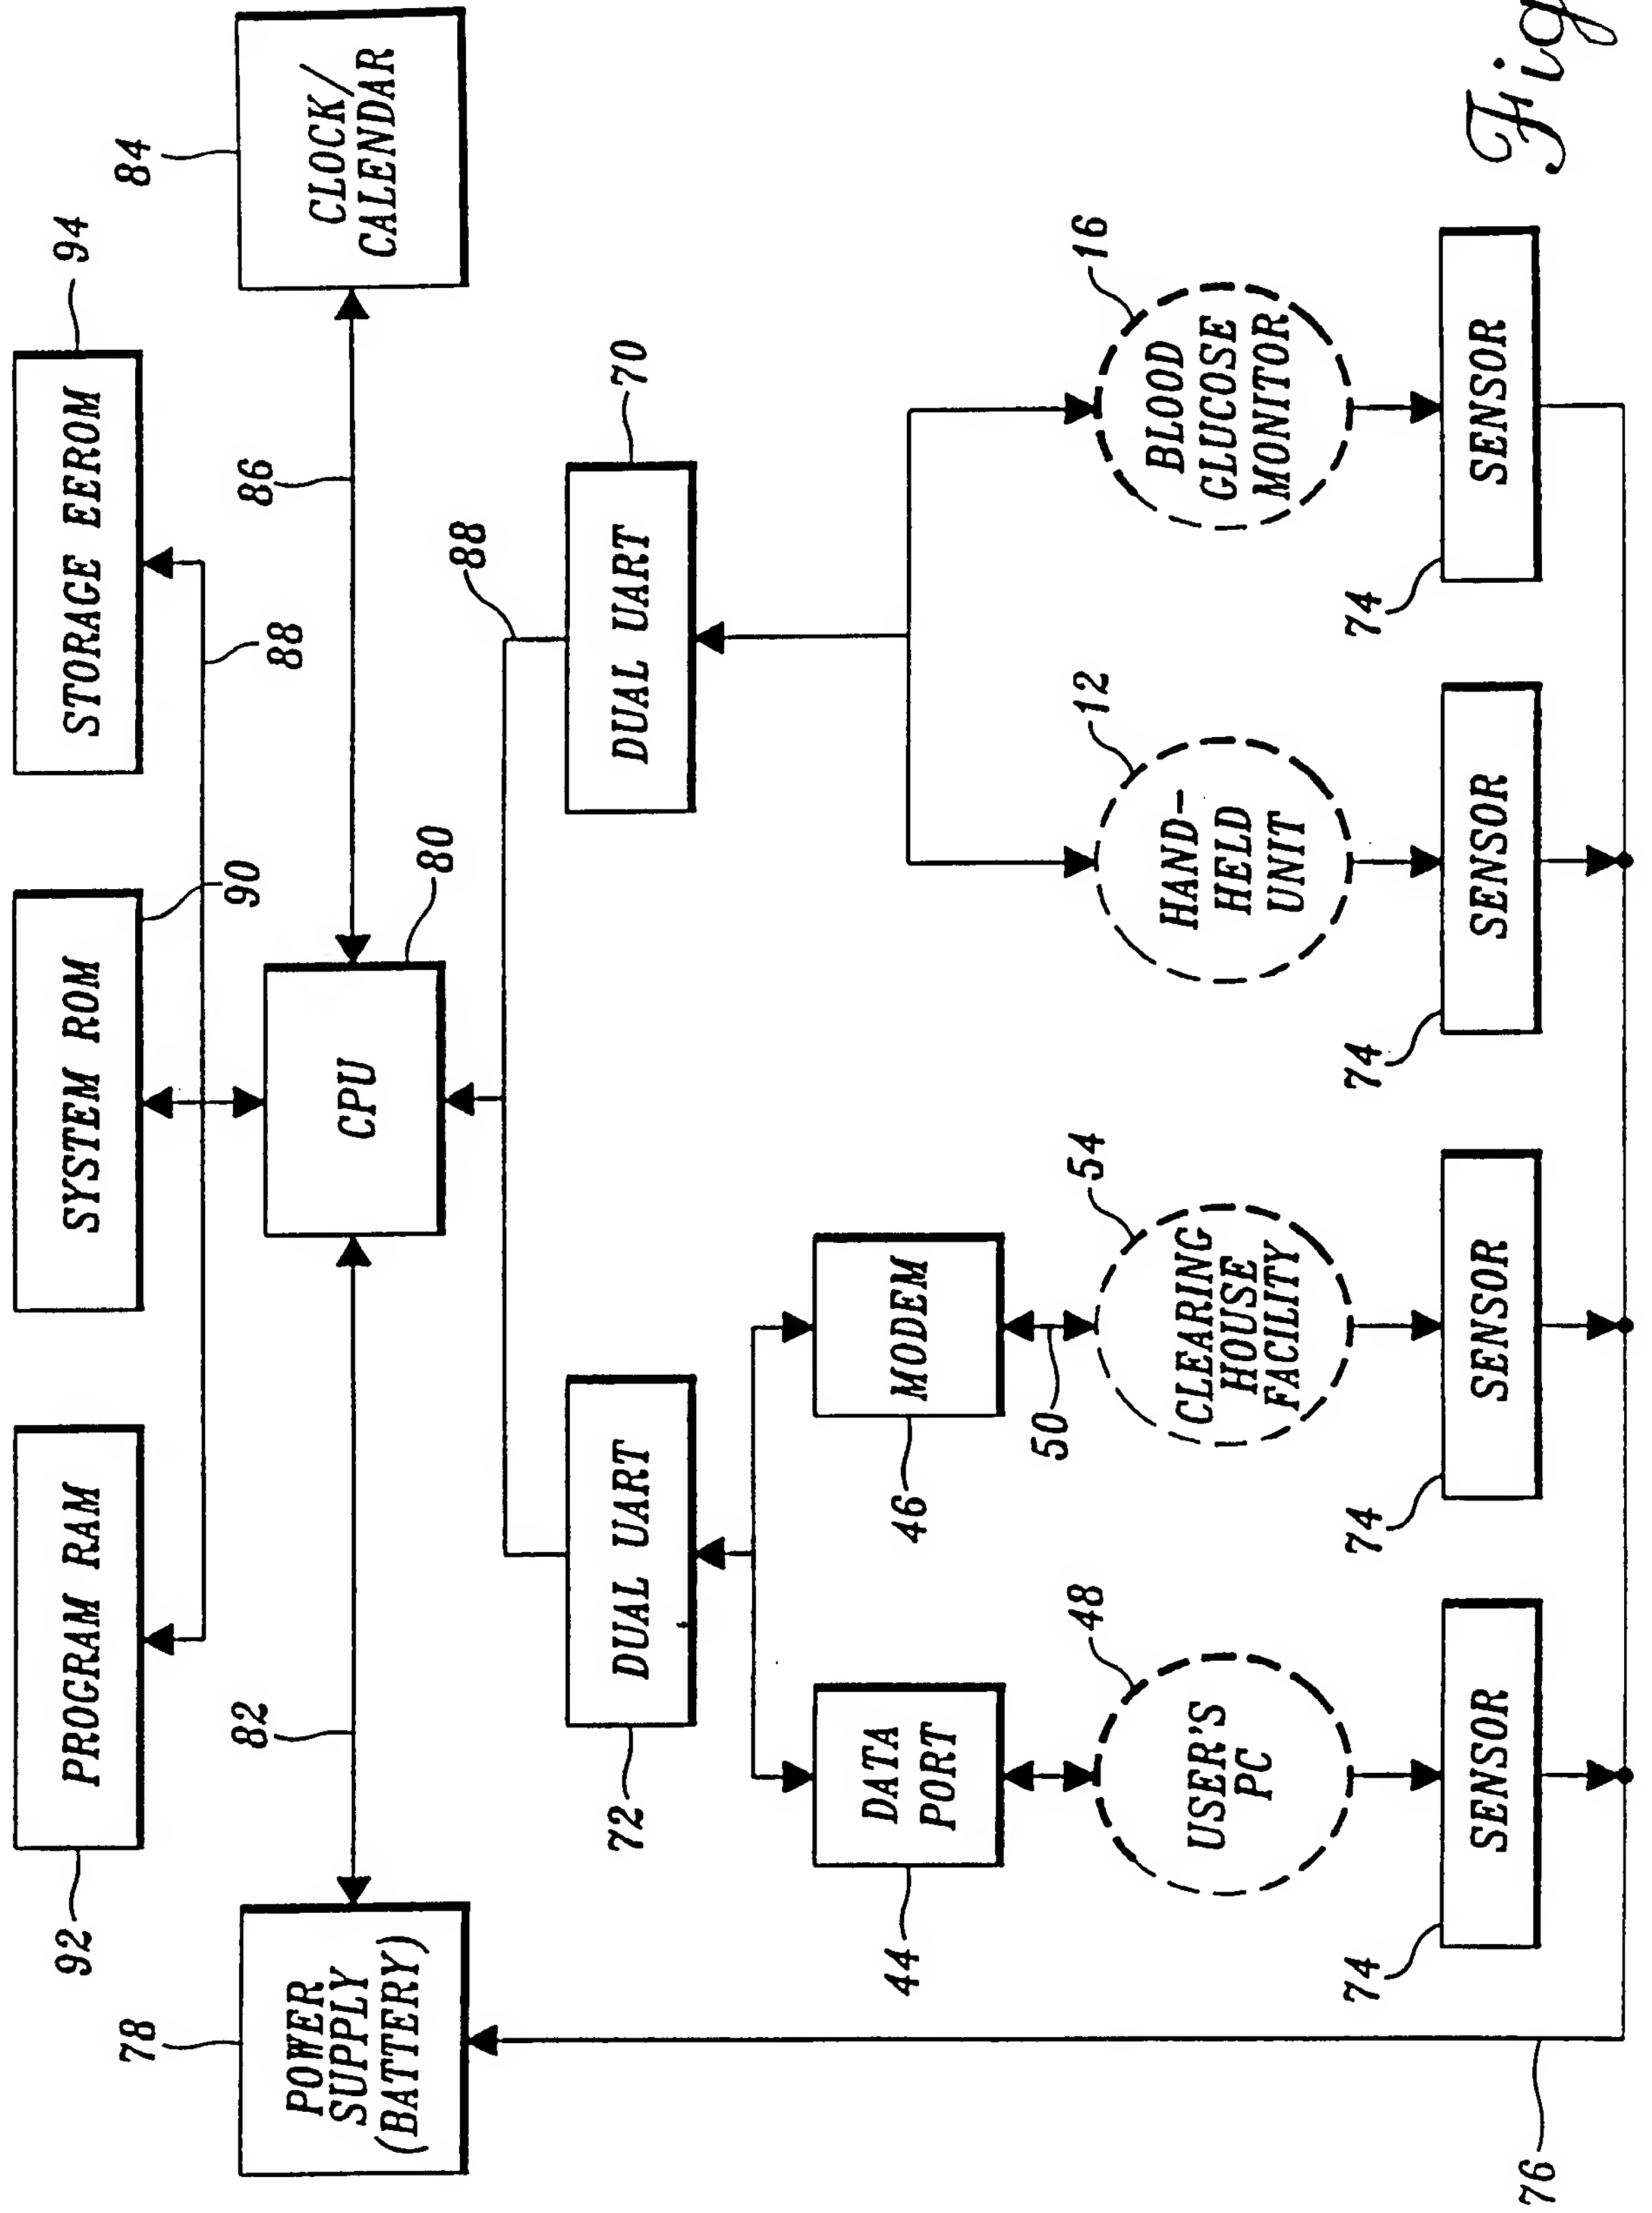


Fig. 3.

*Fig.4.*

**Attention**

Calibration was  
not successful.

Please insert  
the code strip  
again.

*Fig.5.*

June 19 12:30 pm

**Blood Glucose**


**109**

mg /dl

remove test strip

*Fig.6.*

Mon Sept. 28 1992

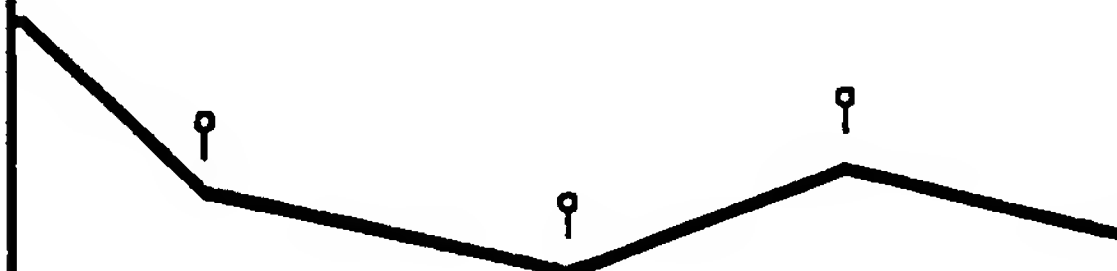


*Fig.7.*


Sept. 20-26 1992



*Fig. 8.*

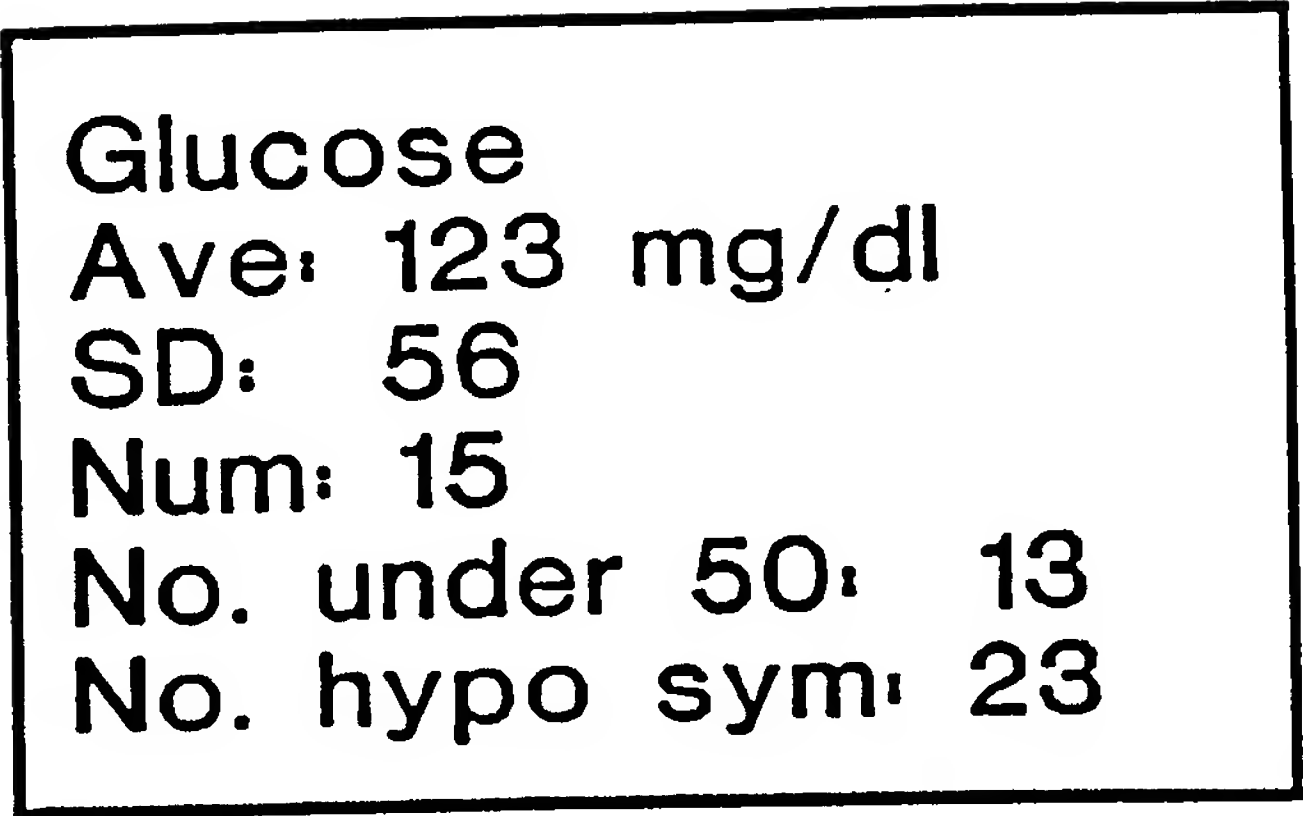

*Fig. 9.*

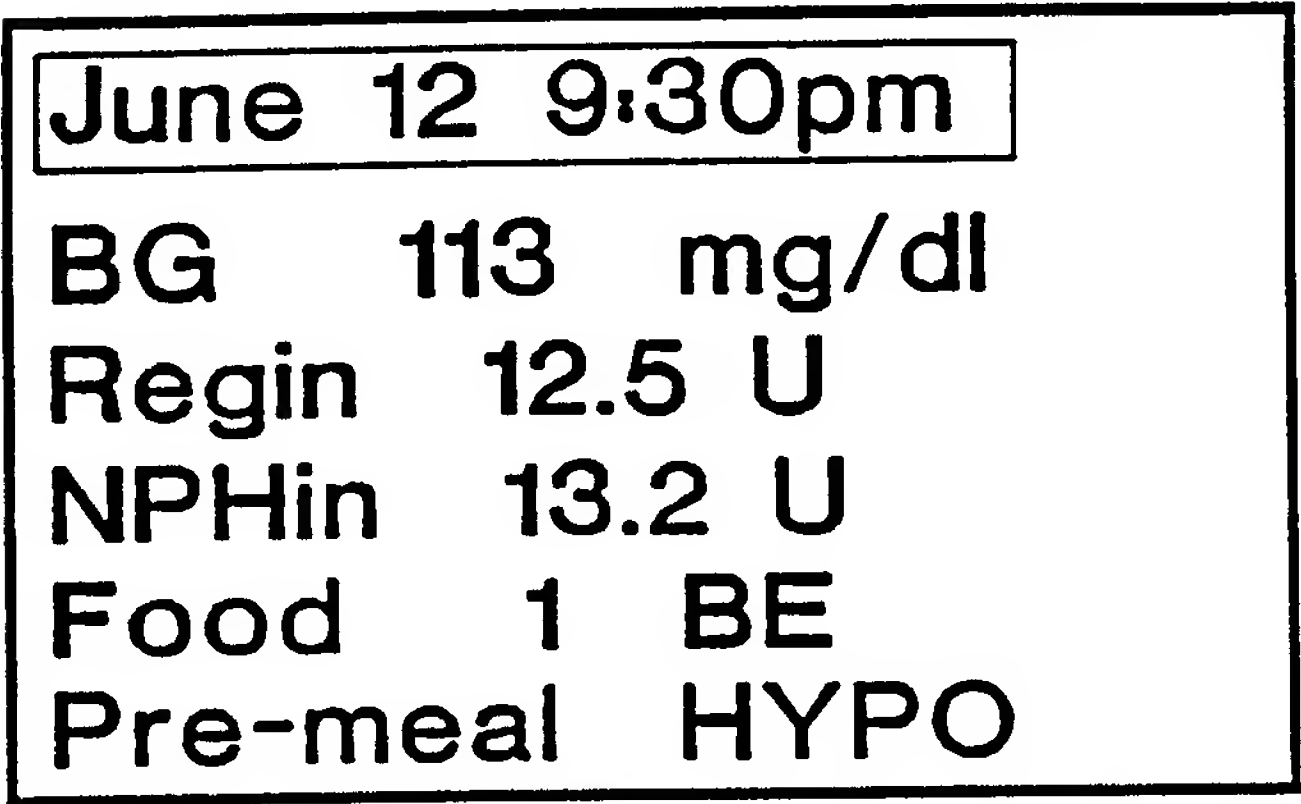

*Fig. 10.*

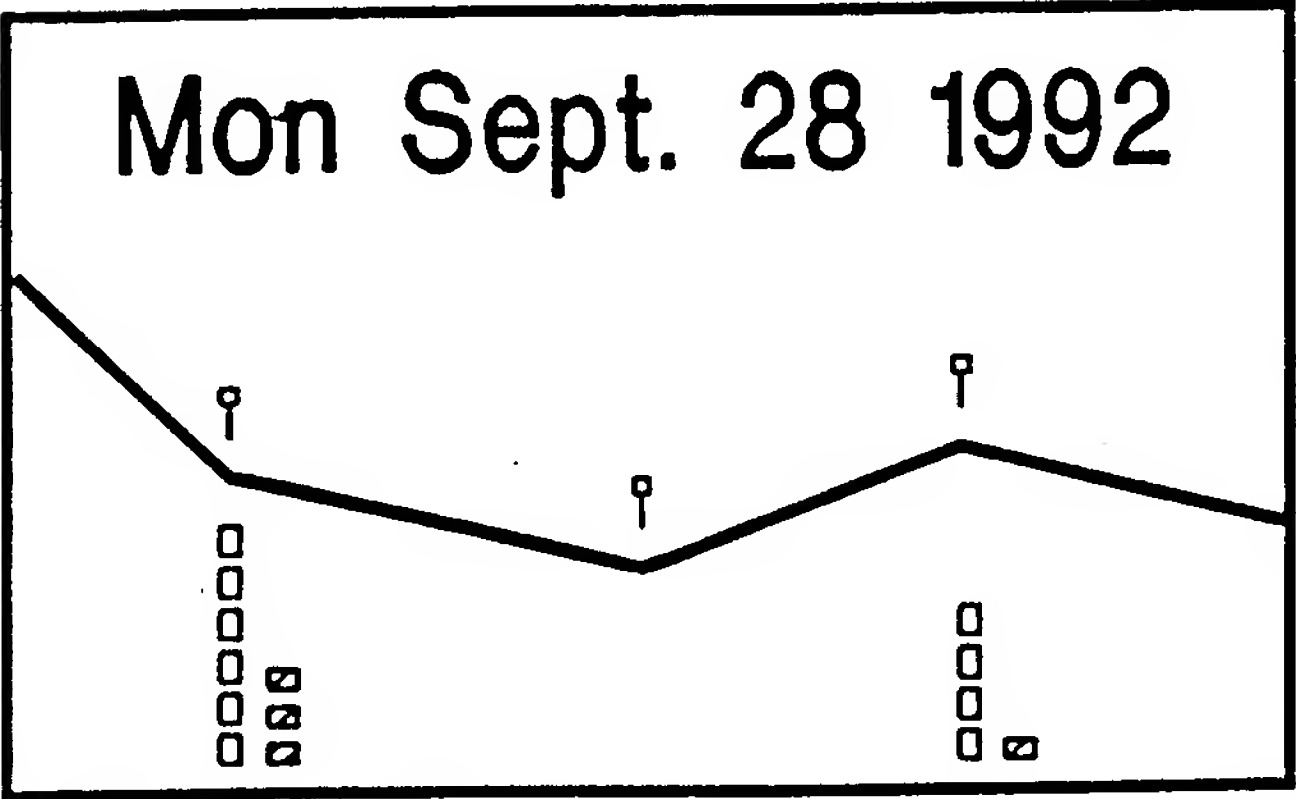


Fig. 11.

